



Fig. 1


Fig. 2

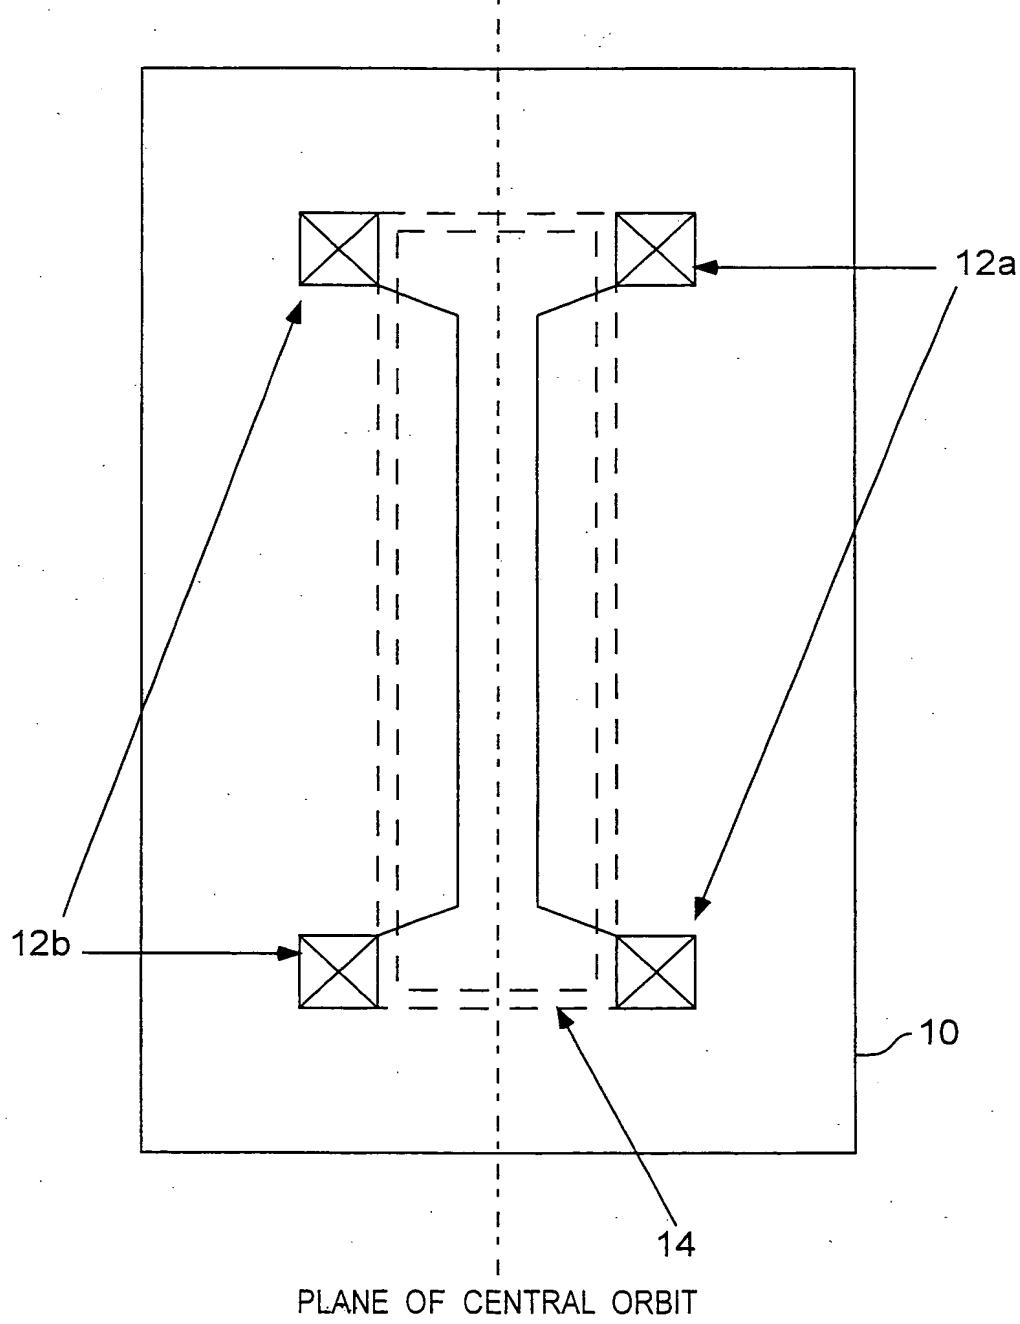

*Fig.3*

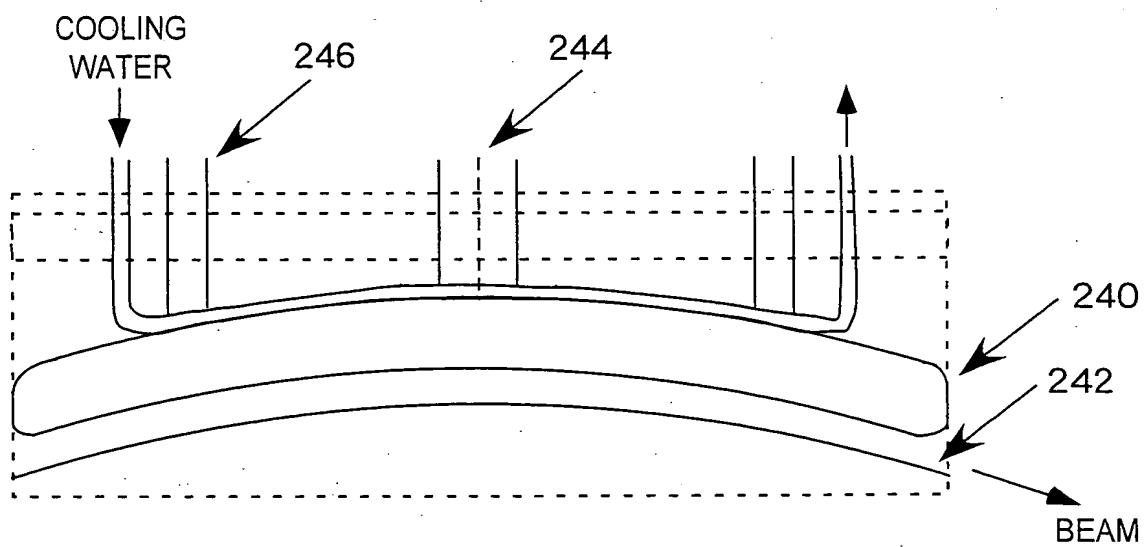


*Fig.4*

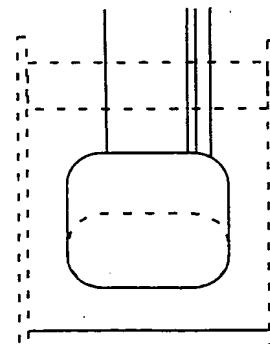

4/8

*Fig.5*

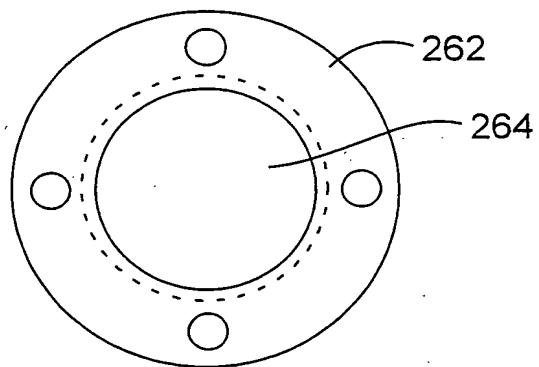

*Fig.6*

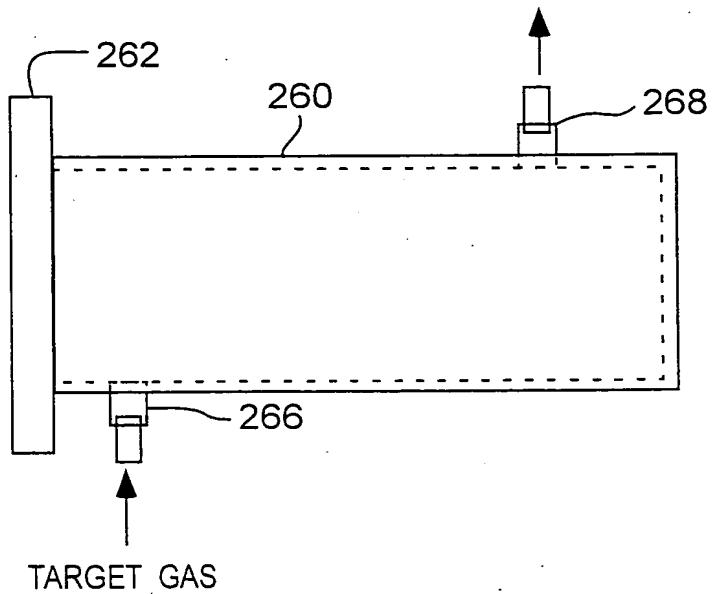


Fig. 7

DOSE EQUIVALENT PER SOLID ANGLE OF DETECTOR  $E_d=3.5$  MeV

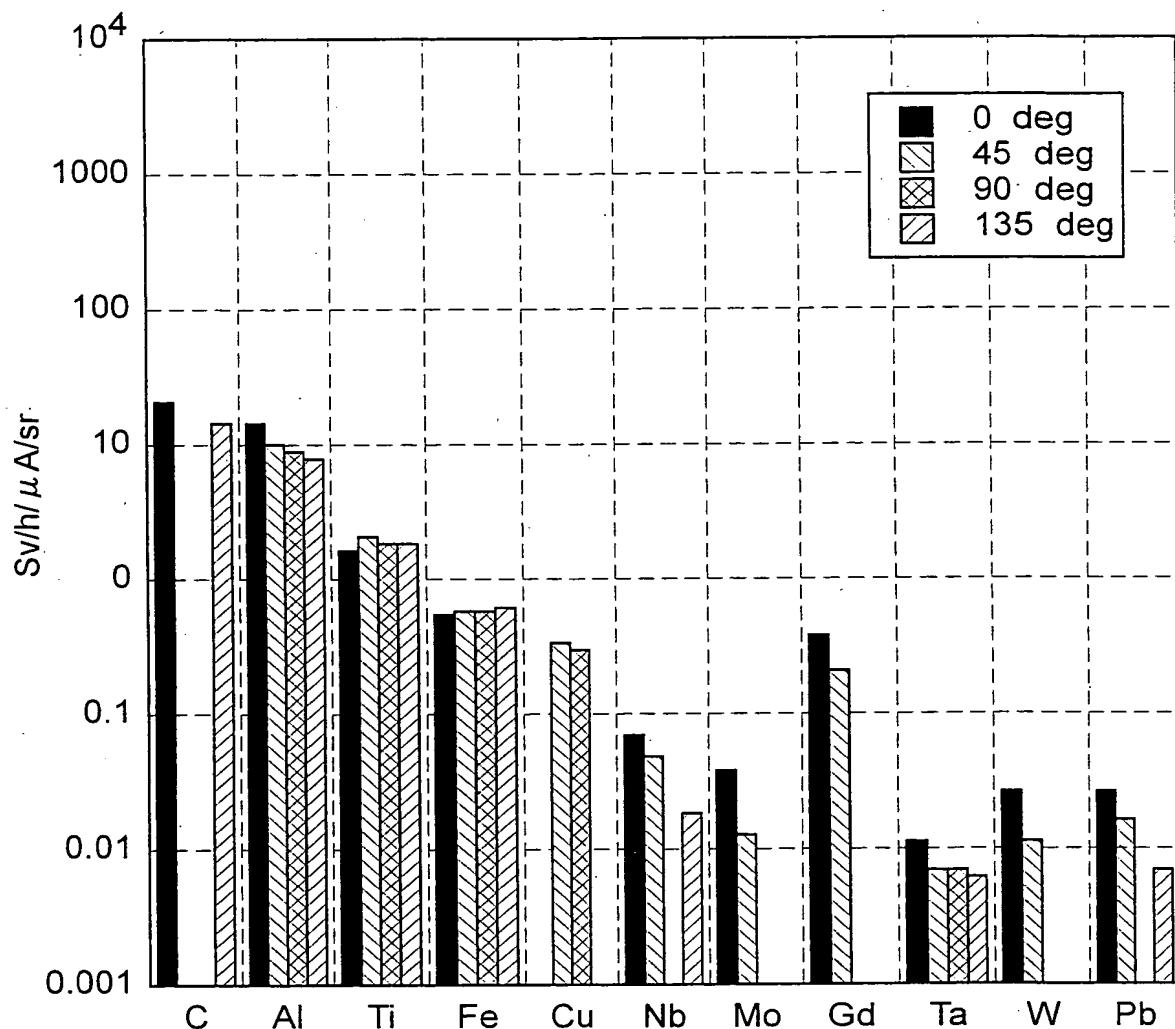


Fig. 8

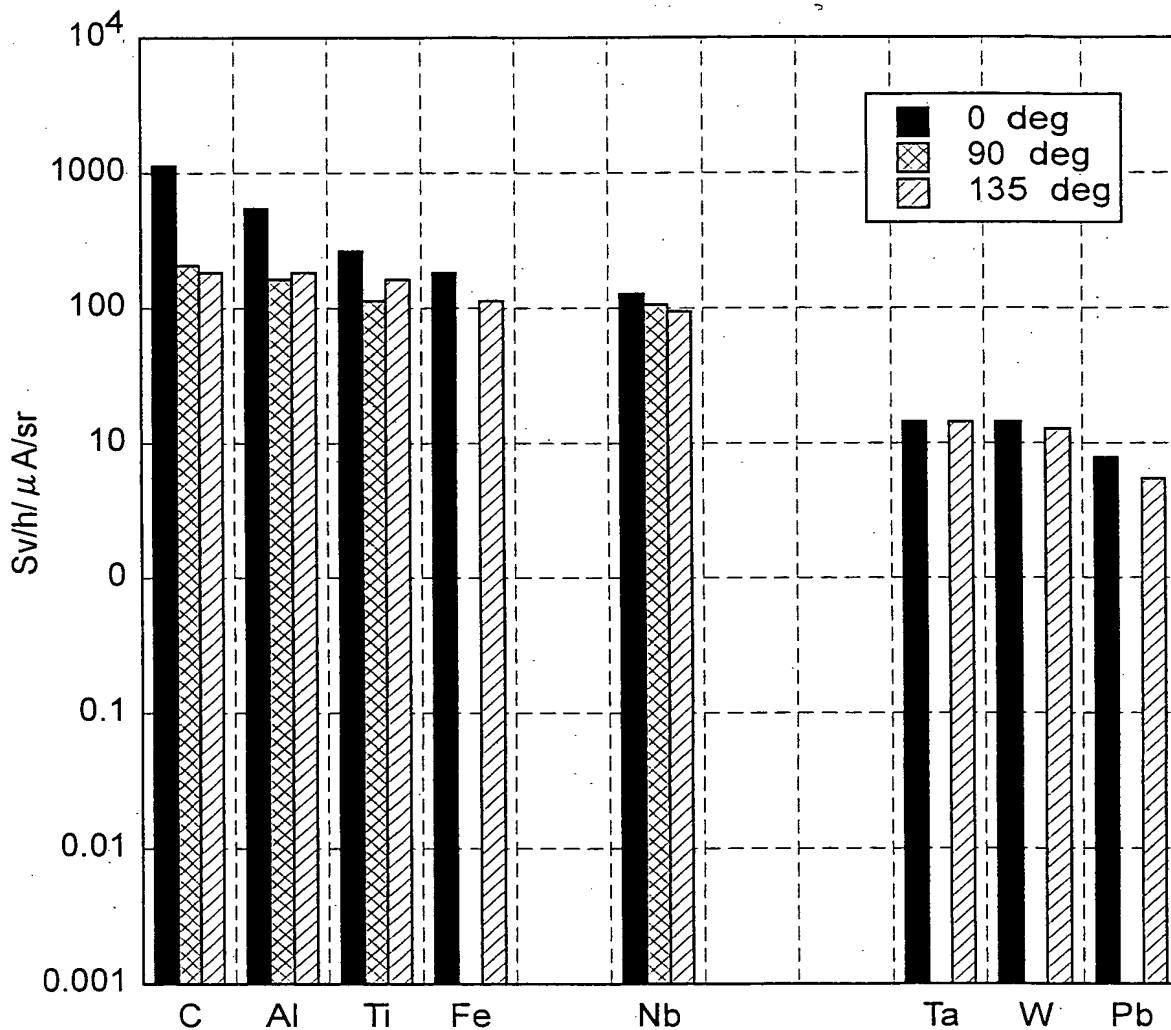
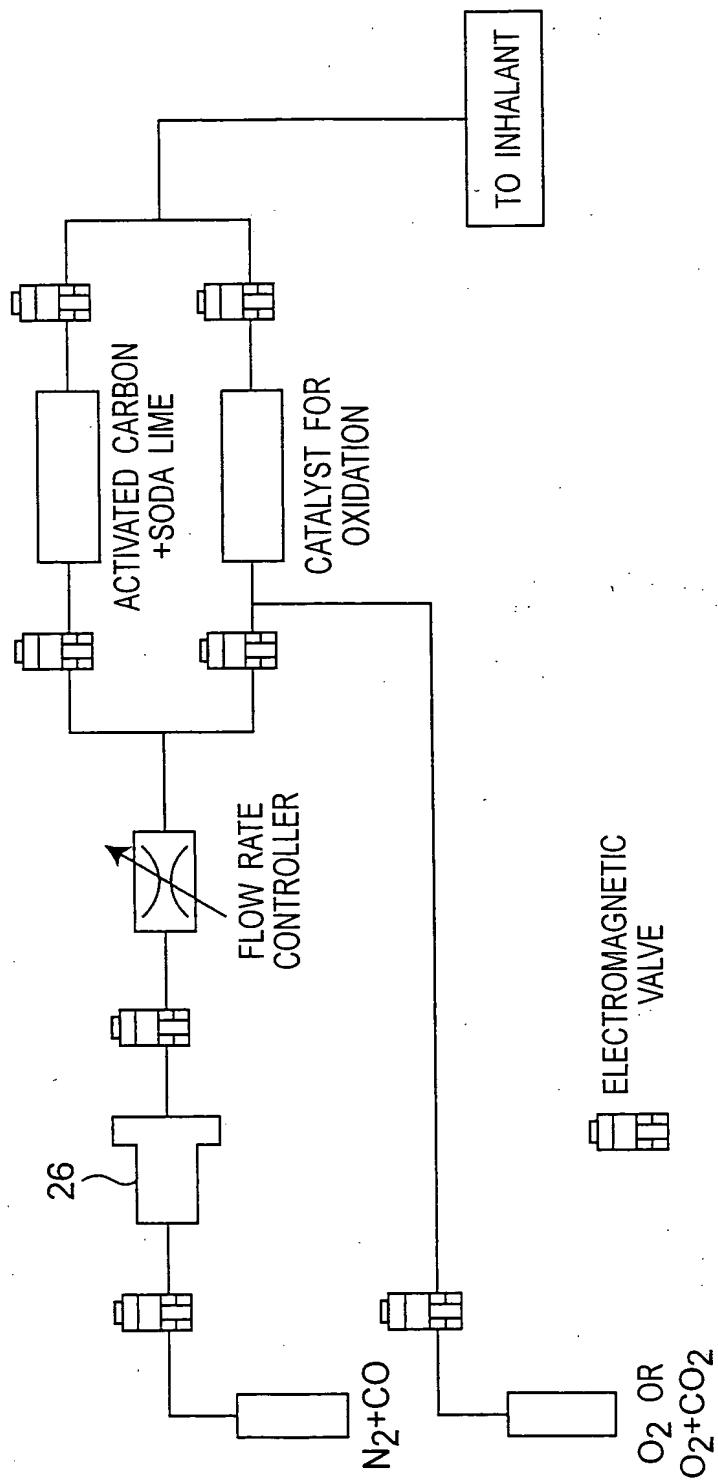
DOSE EQUIVALENT PER SOLID ANGLE OF DETECTOR  $E_d=10$  MeV

Fig. 9



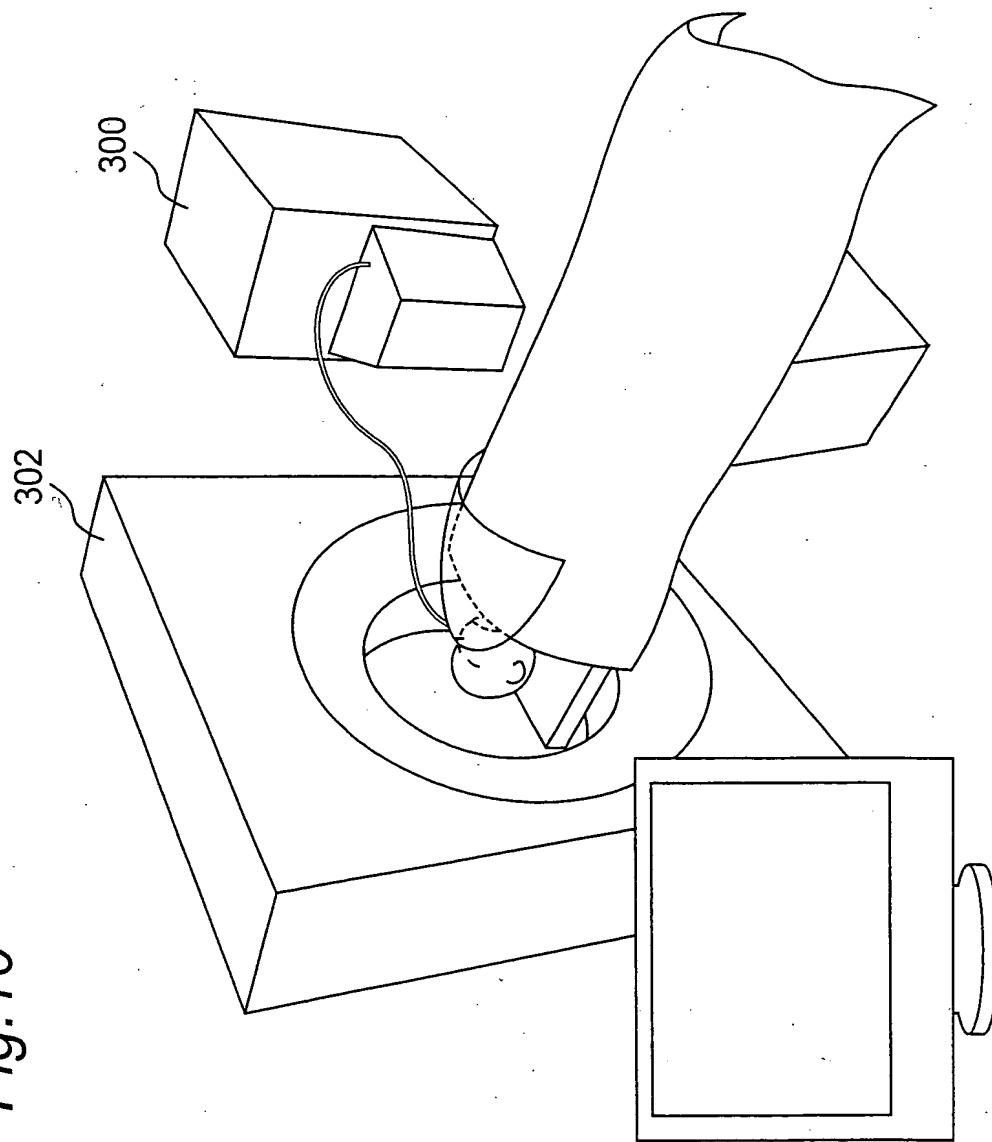


Fig. 10